


Gas chromatography

First instrumental chromatographic method developed commercially.


Reason - it is relatively easy to produce a stable flow and pressure for the mobile phase - **carrier gas**.

All that is really needed is a tank of compressed gas, pressure regulator and a valve.

Schematic of a packed column gas chromatograph

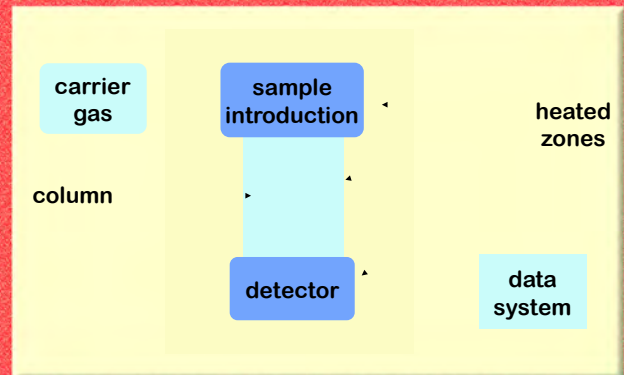

Flow control

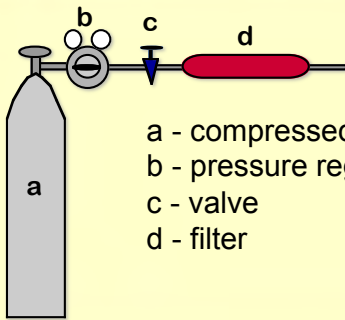

- a - compressed gas cylinder
- b - pressure regulator
- c - valve
- d - filter

Flow measurement

While flow is relatively easy to control, it still must be measured.

Bubble meters - post column or detector measurement of flow. Cheap and relatively accurate.

Rotameters - precolumn measurement of flow via position of ball floating in a calibrated glass tube.

Flow measurement

Electronic flow sensor

A modified thermal conductivity detector.

Permits continuous measurement of flow over a reasonably large range.

Must be calibrated for accurate flow measurement.

Response will also vary based on carrier gas used



Injection methods


With packed column GC, this is a pretty simple portion of the system.

Two basic approaches

Injection ports

Sampling loops / valves

Injection port

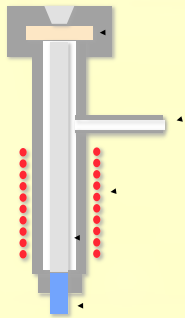

septum

carrier in

heat source

liner

column

Injection port

Purpose of port is to flash evaporate your sample and introduce it into the column.

$$T_{\text{INJ}} > 50^{\circ}\text{C above } T_{\text{column}}$$

Injection is through a septum.

Septum must be
stable at the T_{inj}
replaced regularly to maintain seal

Injection port

Liner.

Provides a known area for the flash vaporization.


Typically made of glass although metal liners may be used. Some instruments don't have liners. Some columns will extend through the port, directly to the septum.

It can and should be replaced at regular intervals - all non-volatile materials and degradation products end up here.

Syringes

Syringes are used to introduce a known volume of a liquid or gas samples .

Adapters can be used to help control the volume injected.

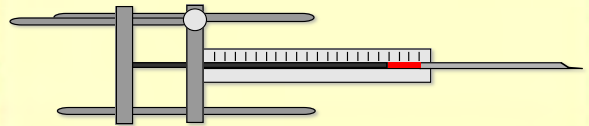

Syringes

Various styles are available

- Fixed needle
- Removable needle
- Several needle lengths and angles


- Sample volumes from $< 1 \mu\text{l}$ and up
- Body loading
- Through the barrel plungers

Syringe filling



When filling, you must insure that there is no air in the syringe.

Syringe injection

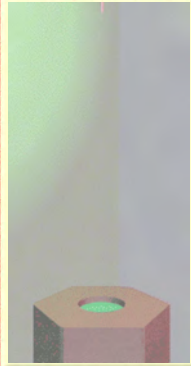

Samples must be injected rapidly so that your sample is introduced as a small 'plug.'

By pulling back on the syringe after injection, you can measure how much sample remains in the needle.

Sample size

Liquids

0.1 - 10 μl is typical

Gases

0.5 - 5 ml is typical

Injection precision with a syringe is +/- 1%


Gas sampling loops

Introducing a constant amount of a gas can be difficult with a syringe.

Gas sampling loops and valves offer a high precision (+/- 0.1%) means of introducing gases.

Equipment is relative inexpensive and only requires a constant temperature for easy use.

Sampling loops

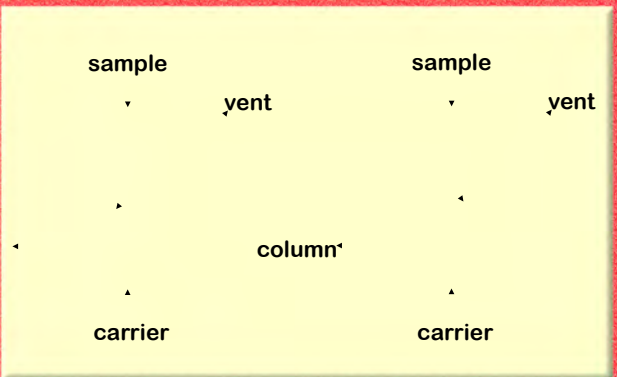

Columns

- Heart of the separation process.
- Vast number of materials have been evaluated.
- It is usually best to refer to various catalogs as an up to date reference.
- Can be classified by tubing diameter and packing type.

Types of columns

Conventional

1/8-1/4" OD, stainless steel or glass tube
6 - 20 feet in length

Preparative

> 1/4"
>10 feet in length

Capillary

0.1 - 0.5 mm ID
10 - 100 meters in length

Types of columns

Columns

Packed

porous packing

non-porous packing

Packed with porous layer

liquid coated

packed capillary

Open tubular (capillary)


coated with porous layer

bound phase

liquid coated wall

Types of columns

Packed




● bead column


● porous layer

● conventional

open (capillary)



Porous Layer Open Tube



Wall Coated Open Tube

Packed vs. capillary columns

	Packed	Capillary
length, M	0.5 - 5	5 - 100
ID, mm	2 - 4	0.1 - 0.7
flow, ml/min	10 - 60	0.5 - 15
head pressure, psig	10 - 40	3 - 40
total plates	4000	250,000
capacity	10 μ g/peak	100ng/peak
film thickness, μ m	1 - 10	0.1 - 8

Improved sensitivity

Because peaks remain narrower, the sensitivity is improved.

Packed

Both peaks have an area of 5000 units.

Capillary

Because the capillary peak is higher, you get a better S/N.

Capillary columns

Available in two basic forms

Coated - simple coating on the inside of a fused silica tube

Bonded - chemically bound via a silane bond.

Both types are coated on the outside with a polyamide to reduce breakage.

Column selection

Unless you're developing new packing materials or methods, the best starting point is to consult a chromatographic catalog.

They provide a wealth of information regarding cost, temperature limits, sample applications.

Another factor to consider, you must use the proper column called for by the 'standard' method (Ex. A specific EPA method.)

Temperature programming

The column sits in an oven.

If the temperature is held constant during the entire analysis it is **isothermal**.

If you vary the temperature during the analysis, you typically use a **temperature program**.

Why bother?


Temperature programming

With homologues, the retention time increases exponentially with the number of carbon.

As t_R increases, width increases and the height decreases, making detection impossible after a few peaks have eluted.

Since solubility of a gas in a liquid decreases as temperature goes up, we can reduce the retention of a material by increasing T_{column} .

Example

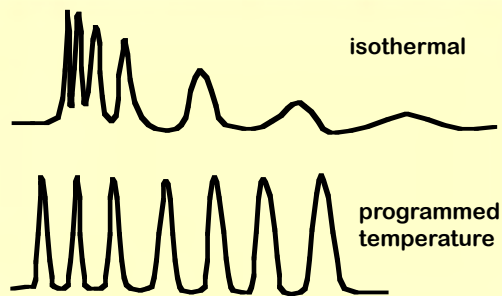

Temperature programming

Factors to consider:

Variations in solubility of solutes

Changes in volatility of solutes

Stability of solutes

Flowrate changes

Stability of stationary phase

Must stay within $T_{\text{min}}/T_{\text{max}}$ of column.

Other factors are found experimentally.

A temperature program

(c)
(b)
(a)

a - initial temperature and time

b - ramp ($^{\circ}\text{C}/\text{min}$)

c - final hold time and temperature

Some GCs will allow for a more complex program.

Temperature programming

General steps to create a program assuming that the separation is possible.

1. Determine initial temperature and time based on best possible separation of first few peaks.
2. Repeat 1 for the last few peaks to find the best final temperature and time.
3. Experiment with various ramps to account for the rest of the components.

Detectors

We need a way to measure our eluents as they evolve from the column.

Virtually every method of directly or indirectly observing eluents as been looked at.

We'll cover some of the more common types.

Detectors

Each can be roughly classified based on

Destructive vs. nondestructive

General vs. some discrimination
vs. very discriminating

Let's start by reviewing some general concepts such as detection limit and sensitivity.

Properties of a good detector

High sensitivity - possible selectivity

Rapidly respond to concentration changes


Large linear range

Stable with respect to noise and drift

Low sensitivity to variations in flow,
pressure and temperature

Produces an easily handled signal

GC detectors sensitivities and ranges

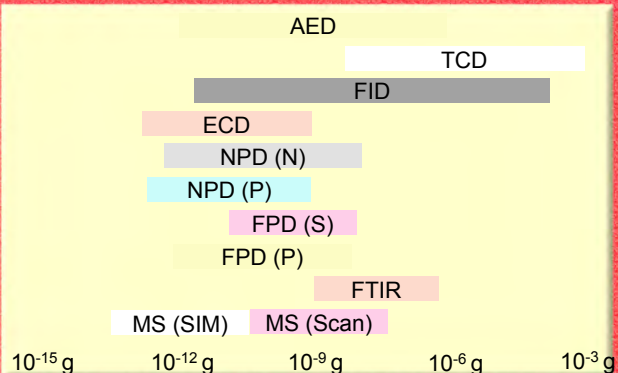

Thermal conductivity detector

General purpose

Nondestructive

Limit of detection ~ 400 pg/ml carrier

Linear range ~ 10⁶

Mode of detection

Change in resistance of a wire based on variations in the thermoconductivity of the gas evolving from a column.

Representative thermal conductivity values, 100°C

Species	Thermal conductivity 10 ⁵ cal/cm sec °C
hydrogen	49.93
helium	39.85
nitrogen	7.18
ethane	7.67
water	5.51
benzene	4.14
acetone	3.96
chloroform	2.33


Thermal conductivity detector

While hydrogen has the largest TC value, helium is commonly used - less reactive.


Hydrogen will give a negative peak when helium is the carrier gas.

Peak response is a function the the TC value for a species so you must standardize for each eluent of interest.

Thermal conductivity detector

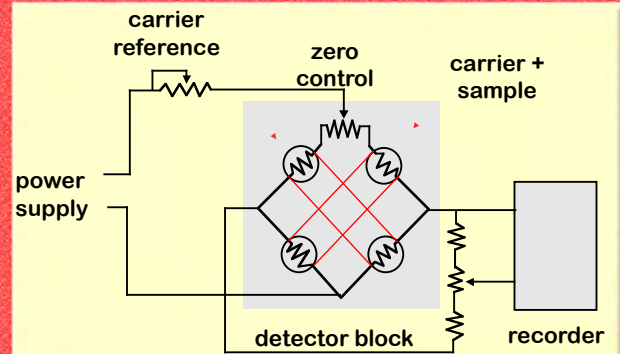

Thermal conductivity detector

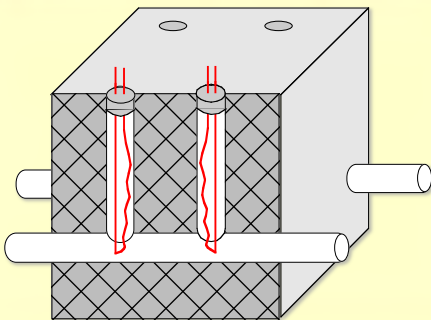

Thermal conductivity detector

Dual channel detectors require both an analytical column and a blank column.

- accounts for response changes due to
 - variations in temperature
 - column bleed

Single channel TCD systems are available that correct for temperature variations.

Flame ionization detector

Specific - sample must be combustible

Destructive

Limit of detection ~ 5 pg carbon / second

Linear range ~ 10^7

Mode of detection

Production of ions in a flame result in a current that can be measured.

A make-up gas may be required to maintain an optimum flow - capillary columns


Flame ionization detector



Sample components enter at the base of the detector. They mix with hydrogen and enter the flame.

Ions are produced that can be measured.

Flame ionization detector

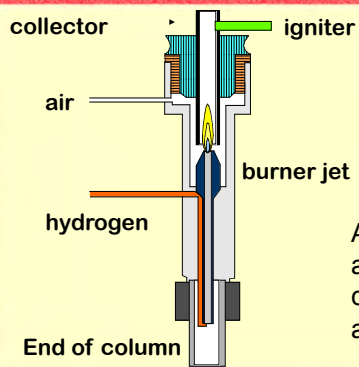

A make-up gas may also be present if capillary columns are to be used.

Flame ionization detector

Compounds with little or no FID response

noble gases	NH ₃	CS ₂
No _x	CO	O ₂
H ₂ O	CO ₂	N ₂

perhalogenated compounds
formic acid
formaldehyde

FID response

Response is based on the number of carbon and if other elements like halogens or oxygen are present which reduce combustion.

formic acid	acetic acid	propionic acid	butanoic acid	pentanoic acid	methane	ethane	propane	butane
-------------	-------------	----------------	---------------	----------------	---------	--------	---------	--------

Electron capture

Specific - sample must contain a gas phase electrophore

Non-destructive


Limit of detection ~ 0.1 pg Cl / second

Linear range ~ 10⁴

Mode of detection

Absorption of β particles by species containing halogens, nitriles, nitrates, conjugated double bonds, organometallics.

Electron capture

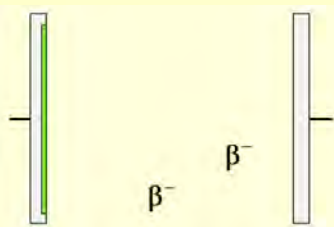


β^- are emitted by an ⁶³Ni source.

Electrophores will absorb β^- , reducing the current.

This is the basis for the response

Electron capture



anode purge vent

anode

⁶³Ni plated surface

makeup gas column

Electron capture detector

Provides excellent trace analysis of

halogenated compounds

nitro group compounds

eluent with conjugated double bonds

Most common use is environmental analysis of organochlorine pesticides

Major problem - detector is radioactive. Requires regular area testing and must be licensed.

Electron capture detector

Relative responses

10^0 hydrocarbons

10^1 esters, ethers

10^2 alcohols, ketones, monochlorides, amines

10^3 monobromides, dichlorides

10^4 anhydrides, trichlorides

10^5 - polyhalogenated, mono and diiodo

10^6